


1

exo

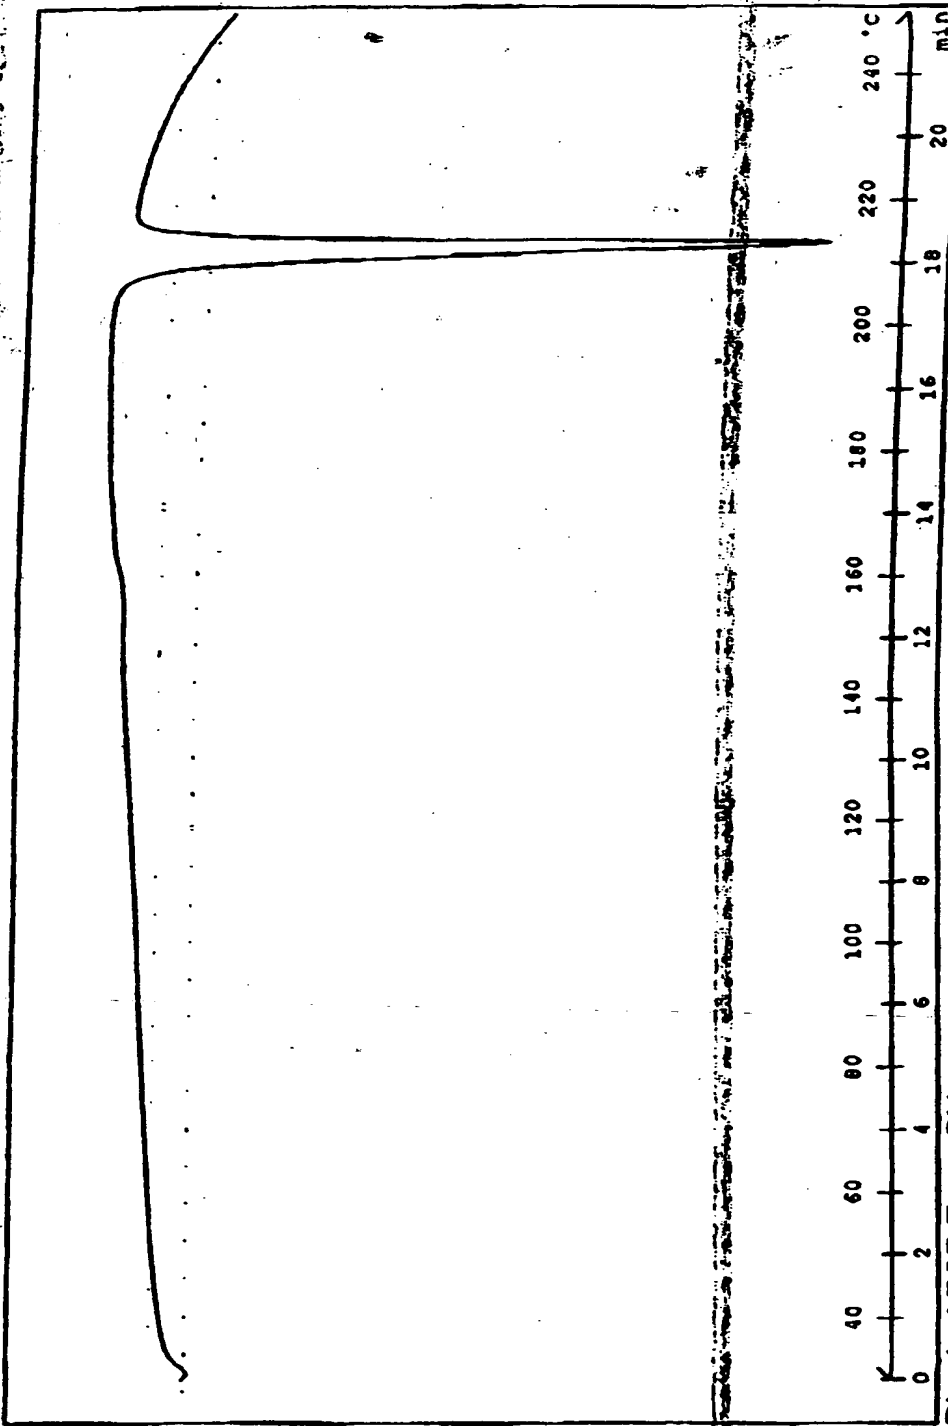

Physical R&D Teva: Shlomo

Figure 1

METTLER TOLEDO STAR System




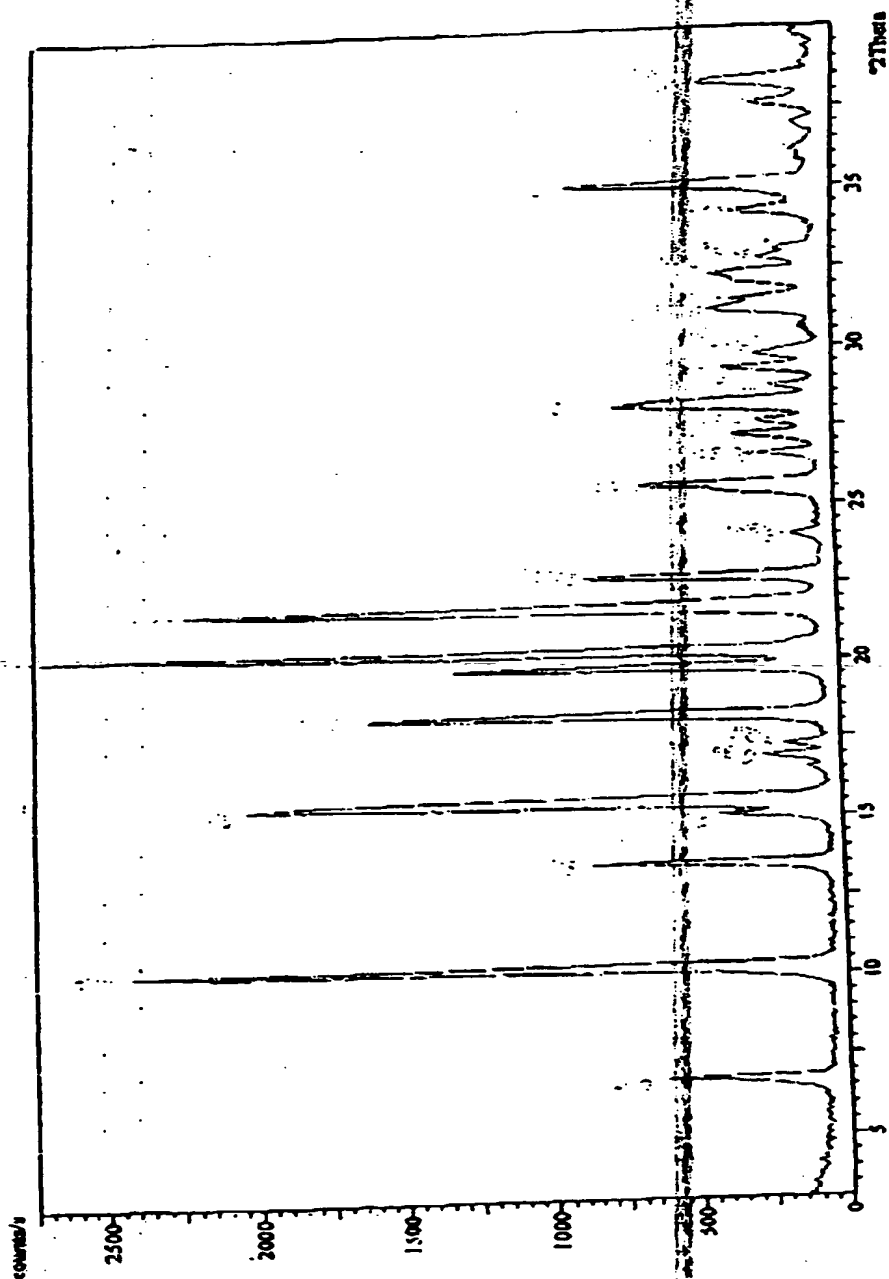


Figure 2



II

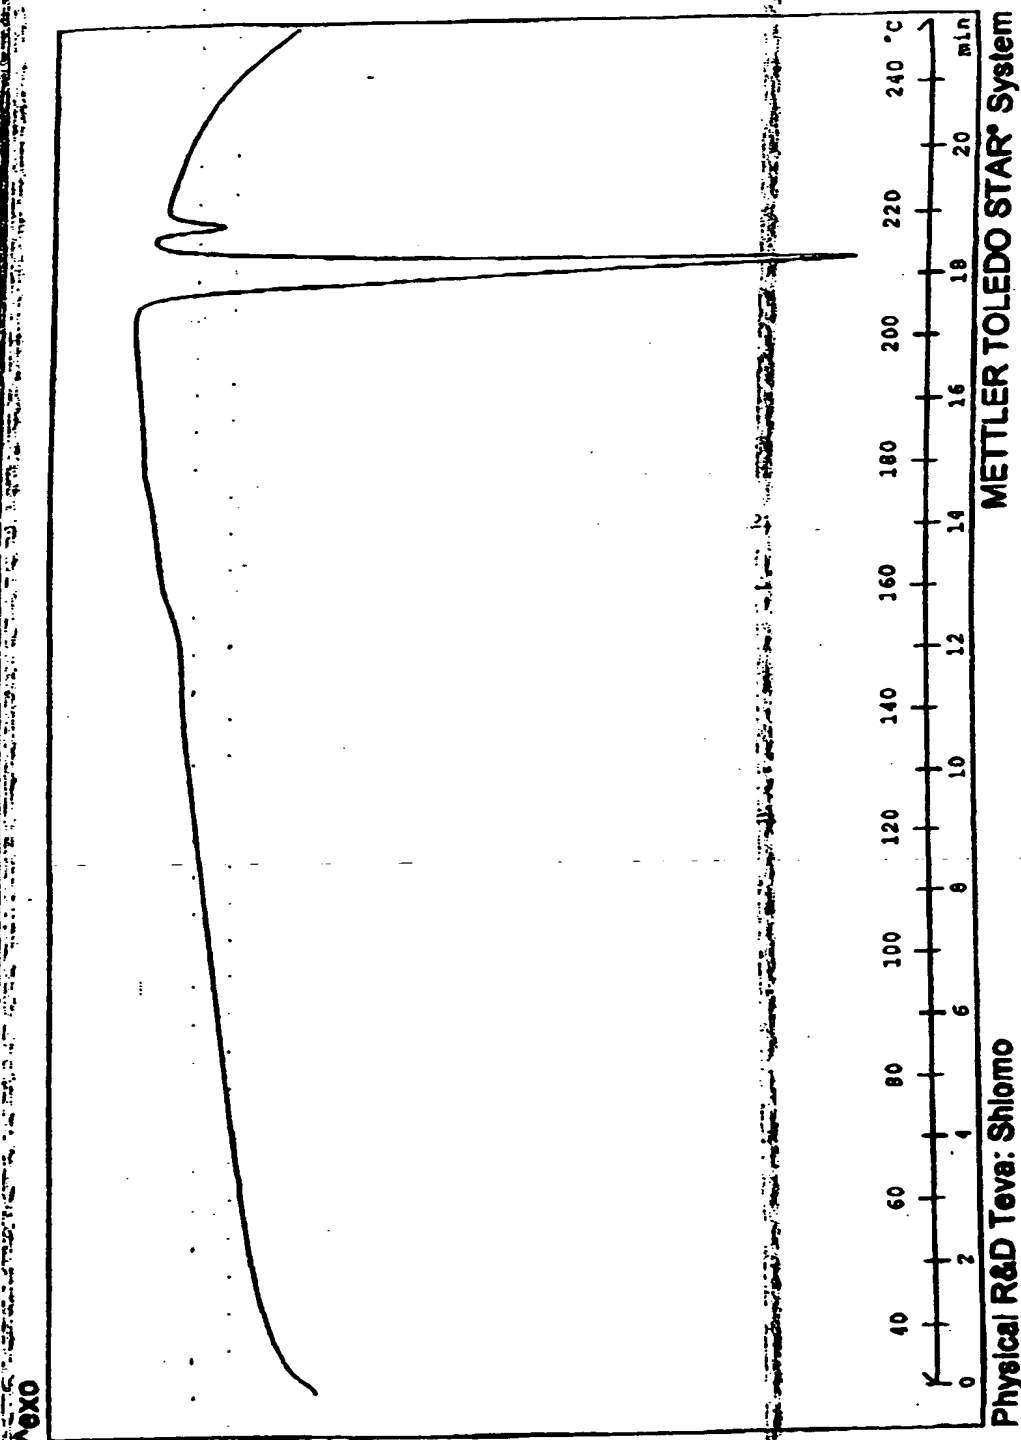


Figure 3



II

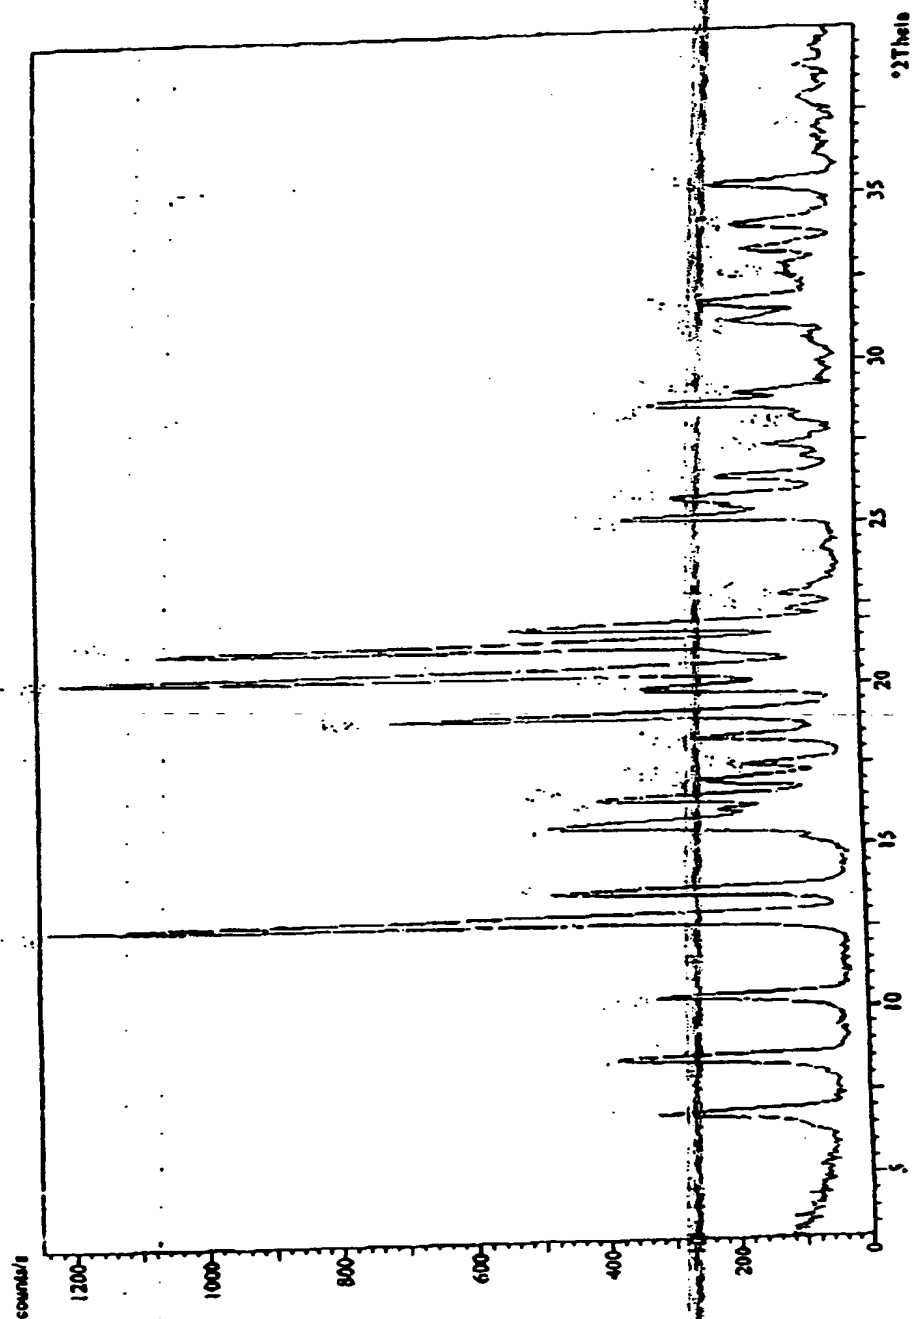
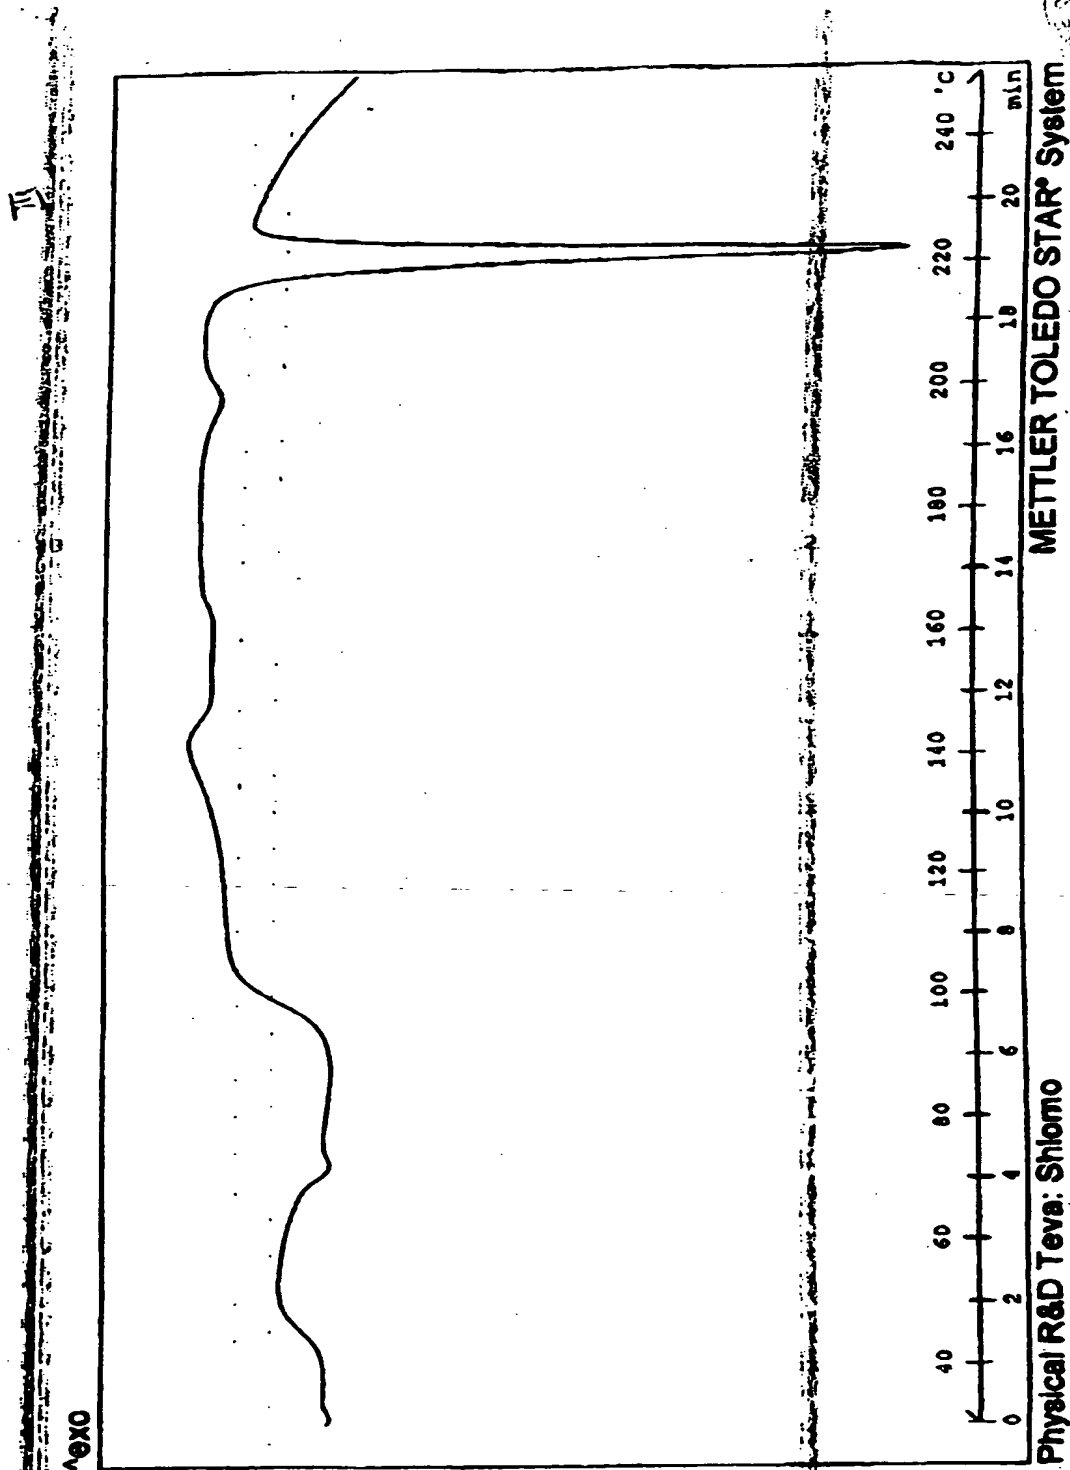


Figure 4




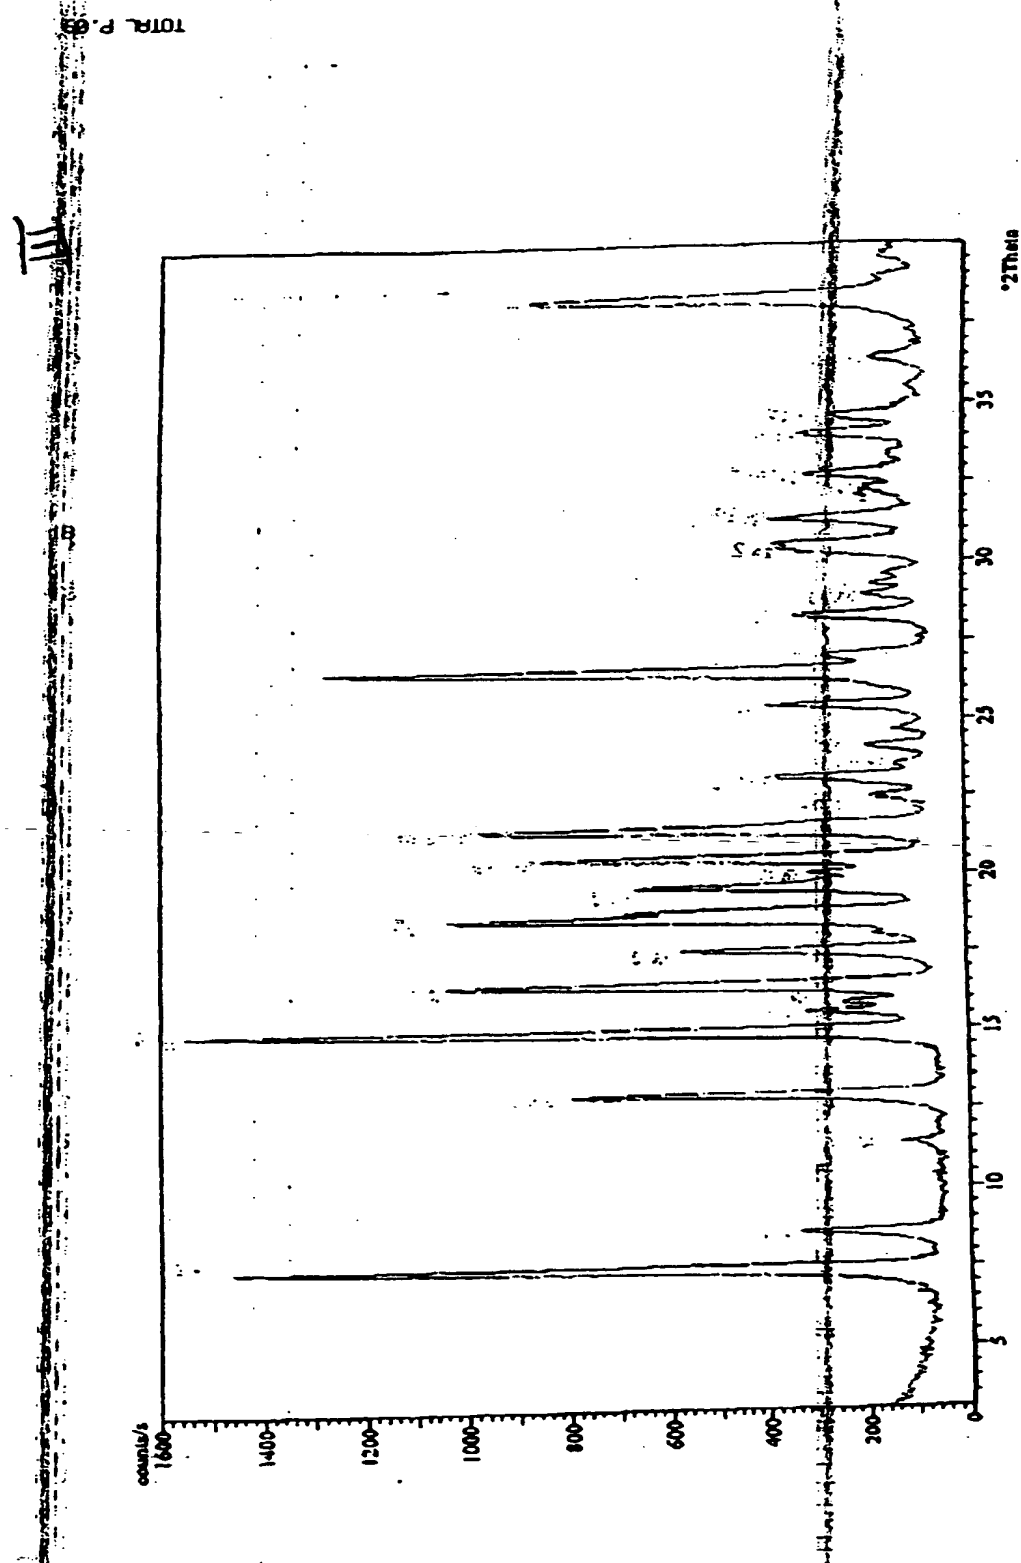


Figure 6

IV

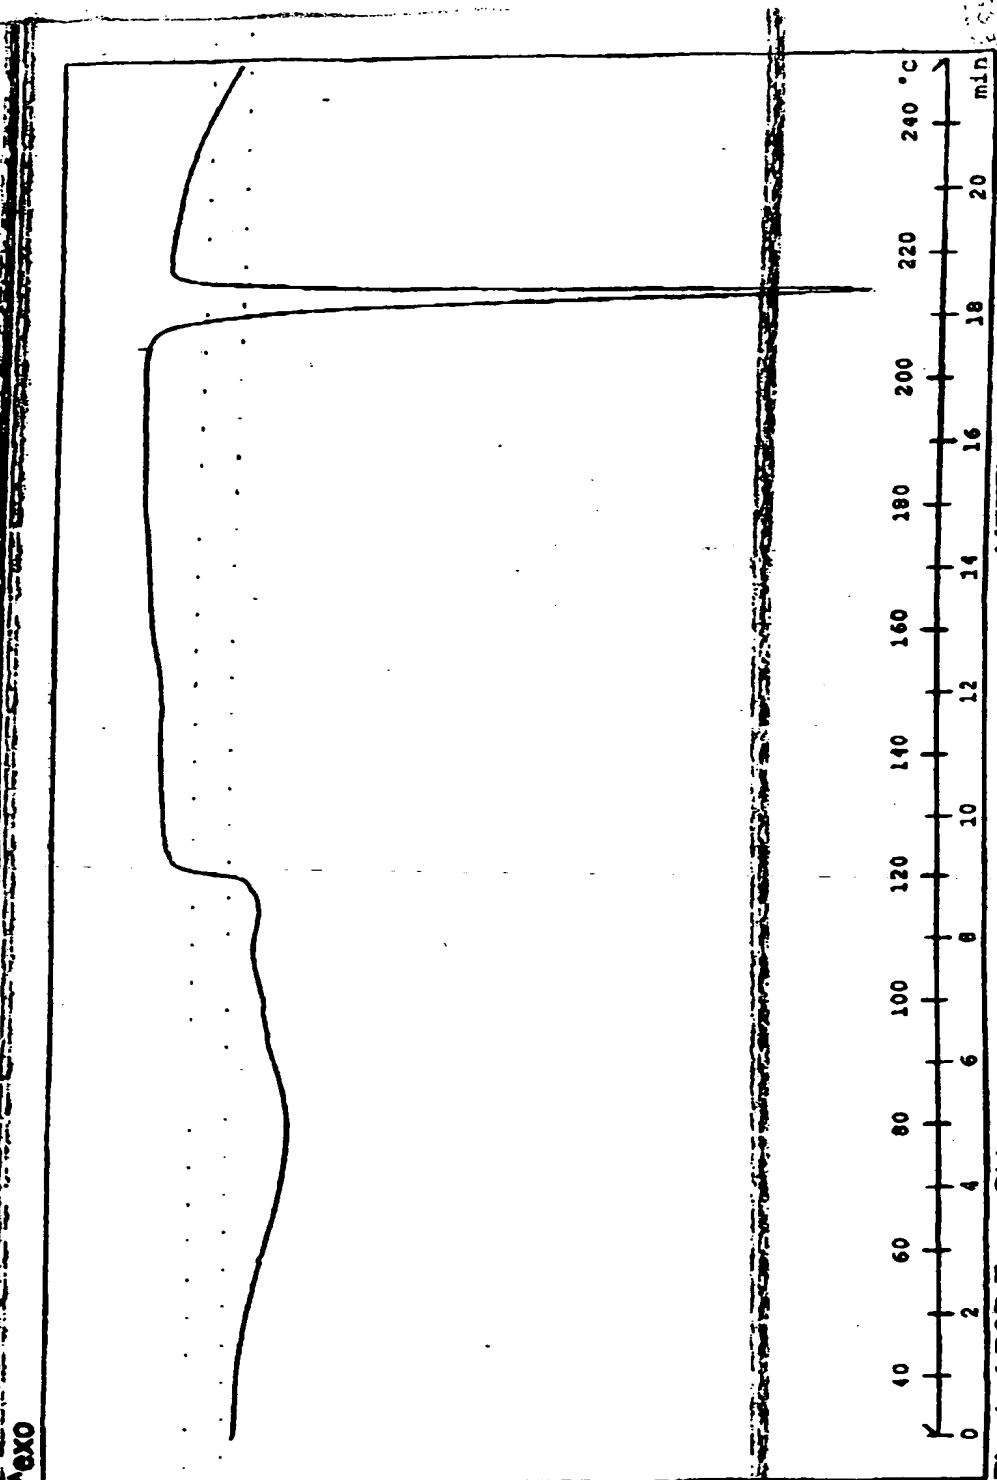

METTTLER TOLEDO STAR System

Figure 7

Physical R&D Teva: Shlomo



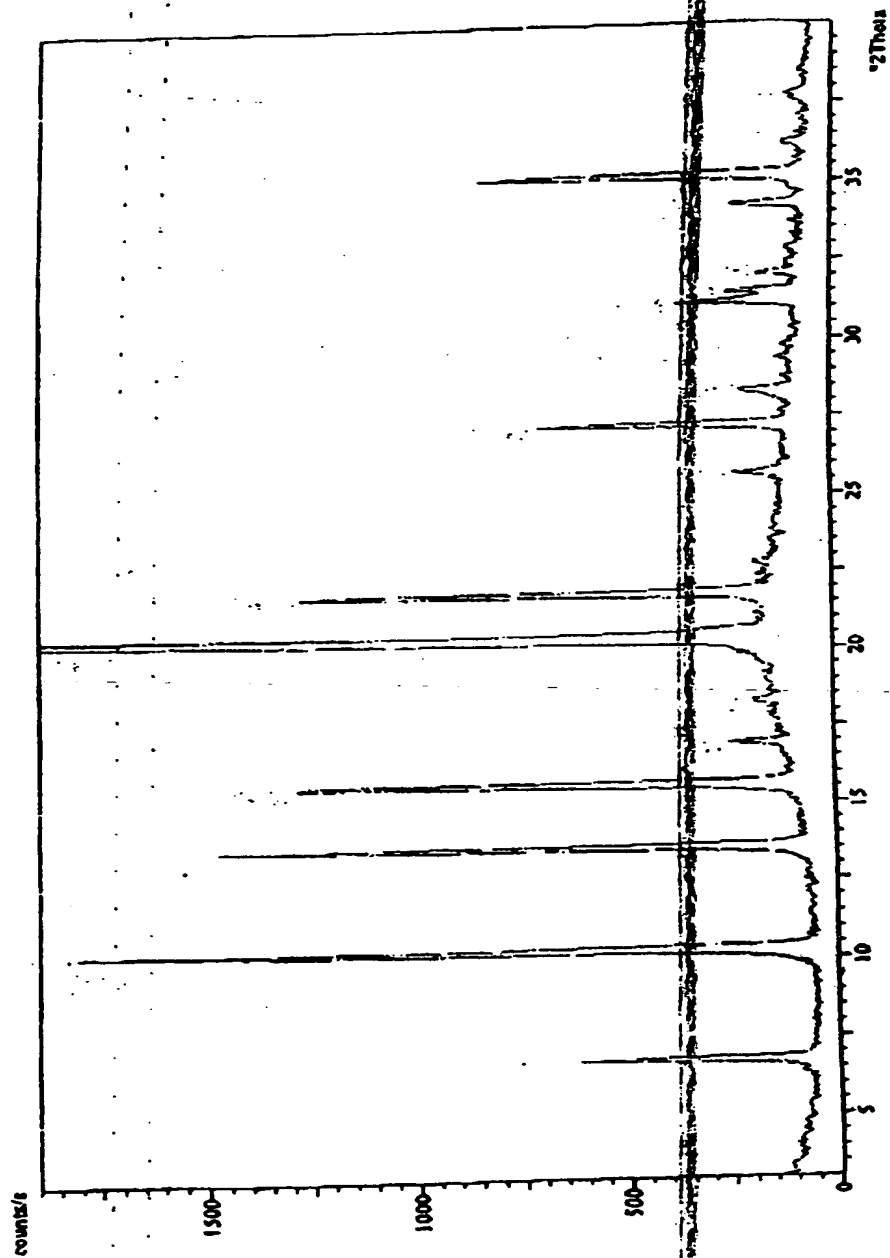


Figure 8

File: VEL-07 SHQ, ID: VEL-07 SHQ.
Date: 02/01/01 13:16 Step: 0.050° Cnt Time: 1.00 Sec.
Range: 2.00 - 40.00 (Deg) Cnt. Scan Rate: 3.00 Deg/min. TEVA

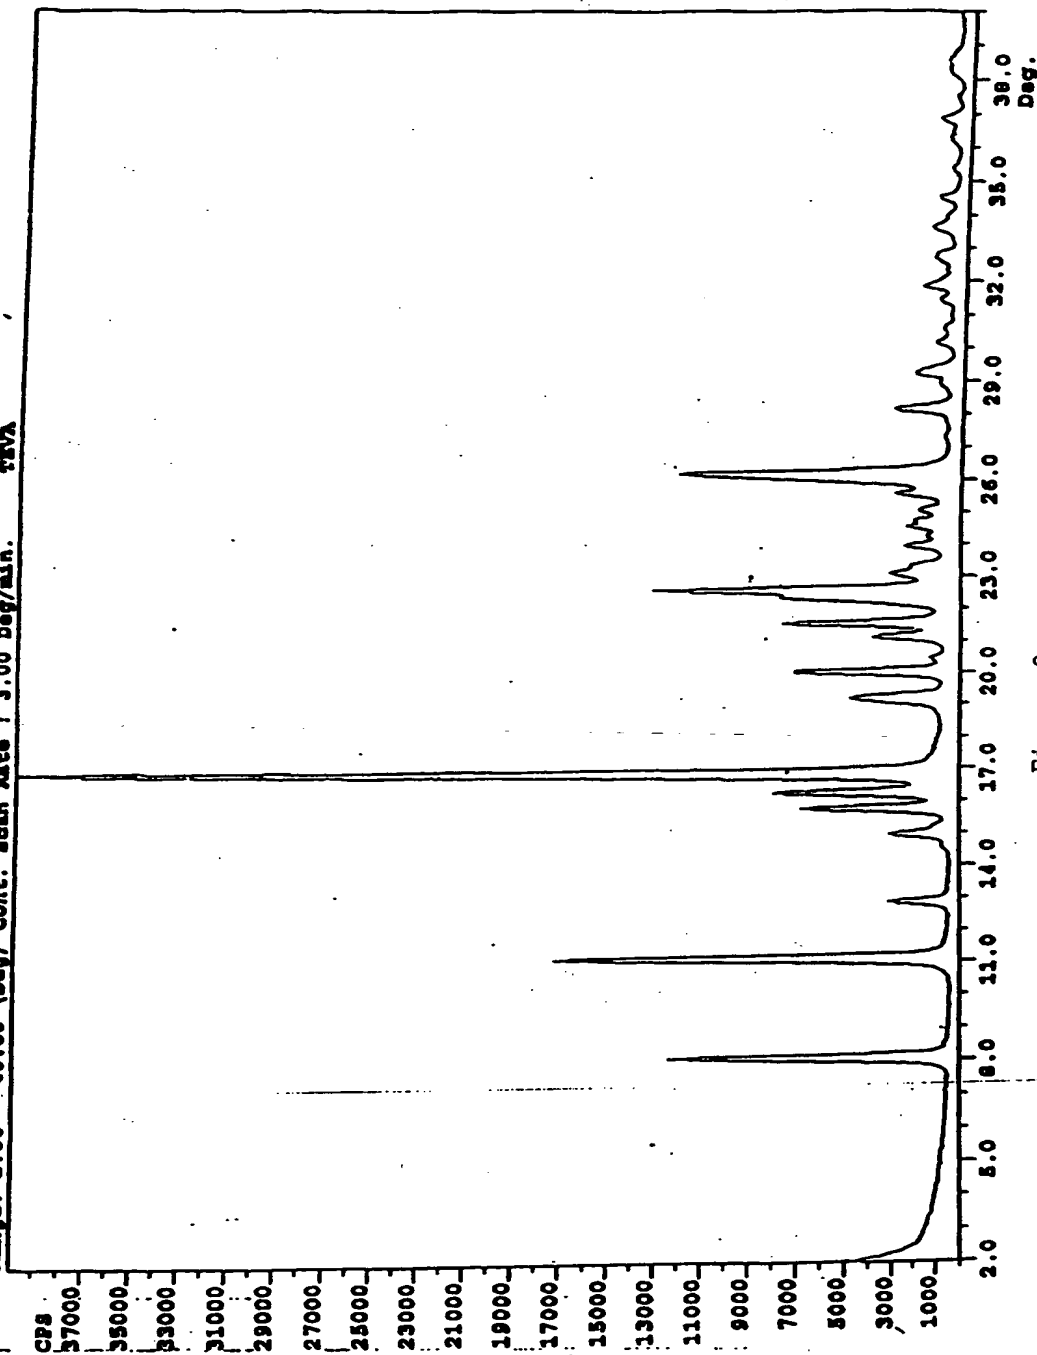


Figure 9

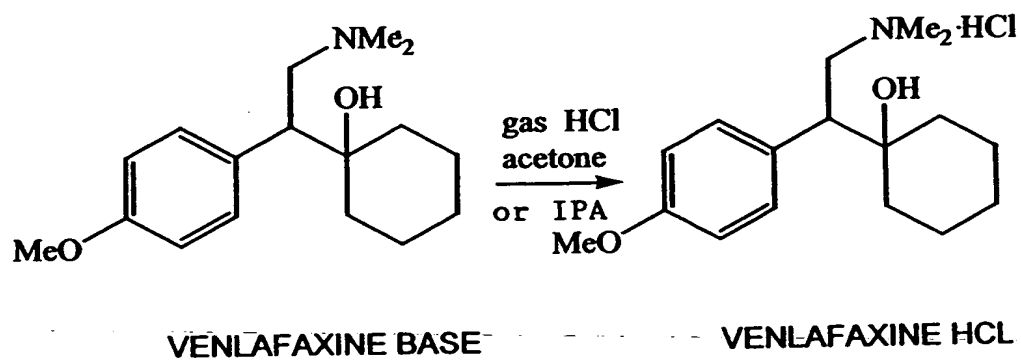


FIGURE 10